

# Mouse IL 1beta ELISA Kit

Mouse IL 1beta ELISA Kit is an Enzyme Immunoassay kit for the quantification of Mouse IL 1beta in serum, plasma and cell culture supernatants.

Catalog number: ARG80196

Package: 96 wells

For research use only. Not for use in diagnostic procedures.

# **TABLE OF CONTENTS**

SECTION	Page
INTRODUCTION	3
PRINCIPLE OF THE ASSAY	3
MATERIALS PROVIDED & STORAGE INFORMATION	4
MATERIALS REQUIRED BUT NOT PROVIDED	4
TECHNICAL NOTES AND PRECAUTIONS	5
SAMPLE COLLECTION & STORAGE INFORMATION	6
REAGENT PREPARATION	7
ASSAY PROCEDURE	9
CALCULATION OF RESULTS	10
EXAMPLE OF TYPICAL STANDARD CURVE	11

## **MANUFACTURED BY:**

Arigo Biolaboratories Corporation

Address: 9F.-7, No. 12, Taiyuan 2nd St., Zhubei City,

Hsinchu County 302082, Taiwan (R.O.C.)

Phone: +886 (3) 621 8100

Fax: +886 (3) 553 0266

Email: info@arigobio.com

### INTRODUCTION

Potent pro-inflammatory cytokine. Initially discovered as the major endogenous pyrogen, induces prostaglandin synthesis, neutrophil influx and activation, T-cell activation and cytokine production, B-cell activation and antibody production, and fibroblast proliferation and collagen production. Promotes Th17 differentiation of T-cells. Synergizes with IL12/interleukin-12 to induce IFNG synthesis from T-helper 1 (Th1) cells. Plays a role in angiogenesis by inducing VEGF production synergistically with TNF and IL6. Involved in transduction of inflammation downstream of pyroptosis: its mature form is specifically released in the extracellular milieu by passing through the gasdermin-D (GSDMD) pore.

# PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for Mouse IL 1beta has been pre-coated onto a microtiter plate. Standards or samples are pipetted into the wells and any IL 1beta present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-conjugated antibody specific for Mouse IL 1beta is added to each well and incubate. Following a washing to remove unbound substances, streptavidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. After washing away any unbound antibody-enzyme reagent, a substrate solution (TMB) is added to the wells and color develops in proportion to the amount of Mouse IL 1beta bound in the initial step. The color development is stopped by the addition of acid and the intensity of the color is measured at a wavelength of 450nm ± 2nm. The

#### Mouse IL 1beta ELISA Kit ARG80196

concentration of Mouse IL 1beta in the sample is then determined by comparing the O.D of samples to the standard curve.

# **MATERIALS PROVIDED & STORAGE INFORMATION**

Upon received, store 100X Antibody Conjugate concentrate at  $\leq$  -20°C. Store other component at 2-8°C at all times. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody Coated Microplate	8 X 12 strips	4°C
Standard	3 vials	4°C
10X Antibody Conjugate Mixture	1.2 ml	≤ -20°C
40X HRP-Streptavidin solution	300 μΙ	4°C
Standard/Sample Diluent Buffer	20 ml	4°C
Antibody Diluent Buffer	35 ml	4°C
10X Wash Buffer	50 ml	4°C
TMB substrate	12 ml	4°C (protect from light)
STOP solution	12 ml	4°C
Plate sealer	4 strips	Room temperature

# MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of reading at O.D. 450 nm
- Centrifuge and centrifuge tube
- Deionized or Distilled water
- Pipettes, pipette tips and Multichannel micropipette reservoir
- Automated microplate washer (optional)

## **TECHNICAL NOTES AND PRECAUTIONS**

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Upon received, store 10X Antibody Conjugate concentrate at ≤ -20°C.
   Store other component at 2-8°C at all times.
- Prior to beginning the assay procedure, bring all reagents and required number of strips to room temperature.
- Briefly spin down the all vials before use.
- If crystals are observed in the 10X Wash Buffer, warm to 37°C until the crystals are completely dissolved.
- Minimize lag time between wash steps to ensure the plate does not become completely dry during the assay.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Take care not to contaminate the TMB Substrate. Do not expose the TMB solution to glass, foil or metal. Do NOT return leftover TMB Substrate to bottle. Do NOT contaminate the unused TMB Substrate. If the solution is blue before use, DO NOT USE IT.
- Change pipette tips between the addition of different reagent or samples.
- Taping the well strips together with lab tape can be done as an extra
  precaution to avoid plate strips from coming loose during the procedure.
- Include a standard curve each time the assay is performed.
- Run both standards and samples in at least duplicates.

# SAMPLE COLLECTION & STORAGE INFORMATION

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

<u>Cell Culture Supernatants -</u> Remove particulates by centrifugation for 10 min at 1500 x g at 4°C and aliquot & store samples at -20°C up to 1 month or -80°C up to 6 months. Avoid repeated freeze-thaw cycles.

<u>Serum -</u> Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Collect serum and assay immediately or aliquot & store samples at-20°C up to 1 month or-80°C up to 6 months. Avoid repeated freeze-thaw cycles.

<u>Plasma - Collect plasma using EDTA or heparin as an anticoagulant.</u> Centrifuge for 15 minutes at 1000 x g. within 30 minutes of collection. Collect the supernatants and assay immediately or aliquot and store samples at -20°C up to 1 month or -80°C up to 6 months. Avoid repeated freeze-thaw cycles.

#### Note:


- Do not use haemolytic, icteric or lipaemic specimens.
- Samples containing sodium azide should not be used in the assay.

### REAGENT PREPARATION

- 1X Wash Buffer: Dilute 10X Wash Buffer into 1X distilled water to yield 1X Wash Buffer (E.g., add 50 mL of 10X Wash Buffer into 450 mL of distilled water to a final volume of 500 mL).
  - The diluted 1X Wash Buffer is stable for 4 weeks at 2°C to 8°C.
- 1X Antibody Conjugate: 20 minutes before use, dilute 10X Antibody
  Conjugate concentrate into Antibody Diluent Buffer to yield 1X Antibody
  Conjugate.
- 1X HRP-Streptavidin Solution: 20 minutes before use, dilute 40X HRP-Streptavidin concentrate into Antibody Diluent Buffer to yield 1X HRP-Streptavidin Solution. Keep diluted HRP-Streptavidin Solution in dark before use.
- Sample: If the initial assay found samples contain IL1 beta higher than the highest standard, the samples can be diluted with Standard diluent buffer and then re-assay the samples. For the calculation of the concentrations this dilution factor has to be taken into account. (It is recommended to do pre-test to determine the suitable dilution factor).
- Standard: Centrifuge the un-reconstituted standard at 6000 x g for 1 minute to bring down the material prior to open the vial. Add 1 ml of Standard / Sample Diluent Buffer to a Standard vial to make the high standard concentration of 1000 pg/mL and brief vortex for few seconds (Do not induce foaming) and allow it to sit for 15 minutes. Make sure the standard is dissolved completely before making serial dilutions. The Standard / Sample Diluent Buffer serves as zero standard (0 pg/ml), and

# **Mouse IL 1beta ELISA Kit ARG80196**

the rest of the standard serial dilution can be diluted with Standard / Sample Diluent Buffer. Diluted the standard as below:

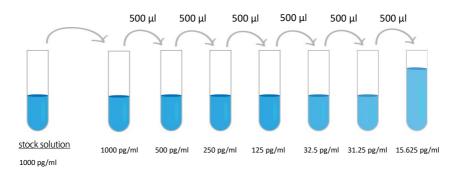

Standard tube	IL 1beta (pg/mL)	Standard / Sample Diluent Buffer (μL)	Standard (μL)
S1	1000	0	1000 (1000 pg/mL Standard Stock)
S2	500	500	500 of S1
S3	250	500	500 of S2
S4	125	500	500 of S3
S5	62.5	500	500 of S4
S6	31.25	500	500 of S5
S7	15.625	500	500 of S6
S0	0	500	0

Note: Working standard should be prepared immediately prior to use.

## **ASSAY PROCEDURE**

All materials should be equilibrated to room temperature (RT, 20-25°C) before use. Standards and samples should be assayed in duplicates.


- 1. Add 100  $\mu$ L of diluted samples or each diluted Standard into respective wells of the 96-well plate.
- 2. Cover the plate and incubate for 1.5 hours at 37°C
- 3. Aspirate each well and wash, repeating the process 4 time for a **total 5** washes. Wash by filling each well with **1X Wash Buffer (300 μL)** using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
- 4. Add 100 μL of 1X Antibody Conjugate to each well.
- 5. Cover the plate and incubate for **1hour** at **37°C**.
- 6. Aspirate each well and wash plate as step 3.
- 7. Add 100 µL of 1X HRP-Streptavidin Solution to each well.
- 8. Cover the plate and incubate for **30 mins** at **37°C** in the dark.
- 9. Aspirate each well and wash plate as step 3.
- 10. Add **100 μL** of **TMB Substrate** in each well.
- 11. Incubate for 15-25 mins at 37°C in the dark.
- 12. Add **100 μL** of **Stop Solution** to each well to stop the reaction.
- 13. Read the absorbance with a plate reader at **O.D. 450 nm.** It is recommended reading the absorbance within 10 minutes after adding the stop solution.

### **CALCULATION OF RESULTS**

- Calculate the average absorbance values for each set of standards, control and samples.
- 2. Using log-log, semi-log or linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
- 3. Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
- 4. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
- 5. arigo provides GainData®, an in-house development ELISA data calculator, for ELISA data result analysis. Please refer our GainData® website for details. (https://www.arigobio.com/elisa-analysis)
- 6. If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.

## **EXAMPLE OF TYPICAL STANDARD CURVE**

The following figures demonstrate typical results with the Mouse IL 1beta ELISA Kit. One should use the data below for demonstration only and cannot be used in place of data generations at the time of assay.

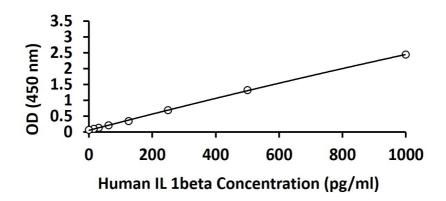

# **QUALITY ASSURANCE**

# Sensitivity

7.8 pg/ml

# **Assay Range**

15.625 - 1000 pg/mL