



Pistachio ELISA Kit

Enzyme Immunoassay for the quantitative determination of Pistachio in food

Catalog number: ARG80811

For research use only. Not for use in diagnostic procedures.

TABLE OF CONTENTS

SECTION	Page
INTRODUCTION	3
PRINCIPLE OF THE ASSAY	3
MATERIALS PROVIDED & STORAGE INFORMATION.....	4
MATERIALS REQUIRED BUT NOT PROVIDED.....	4
TECHNICAL HINTS AND PRECAUTIONS	5
SAMPLE COLLECTION & STORAGE INFORMATION	5
REAGENT PREPARATION	6
ASSAY PROCEDURE	7
CALCULATION OF RESULTS.....	7
EXAMPLE OF TYPICAL STANDARD CURVE.....	8
QUALITY ASSURANCE	9

MANUFACTURED BY:

Arigo Biolaboratories Corporation

Address: No. 22, Ln. 227, Gongyuan Rd., Hsinchu City 300, Taiwan

Phone: +886 (3) 562 1738

Fax: +886 (3) 561 3008

Email: info@arigobio.com

INTRODUCTION

Pistachio (*Pistacia vera*) belongs to the family of Anacardiaceae. With about 21% the fraction of proteins in pistachio seed is very high. Some of these proteins, like the 2S albumin Pis v 1, the 11S globulin Pis v 2 or the 7S vicillin Pis v 3 are known for being allergenic. Many of them are heat resistant making them stable to different production processes. For this reason pistachio represents an important food allergen.

For pistachio-allergic persons hidden pistachio allergens in food are a critical problem. Already very low amounts of pistachio can cause allergic reactions, which may lead to anaphylactic shock in severe cases. Because of this, pistachio-allergic persons must strictly avoid the consumption of pistachio containing food. Cross-contamination, mostly in consequence of the production process, is often noticed. This explains why in many cases the existence of pistachio residues in food cannot be excluded. For this reason sensitive detection systems for pistachio residues in food-stuffs are required.

PRINCIPLE OF THE ASSAY

This assay employs the sandwich quantitative enzyme immunoassay technique. An antibody directed against pistachio proteins is bound on the surface of a microtiter plate. Pistachio proteins containing samples or standards are given into the wells of the microtiter plate. After 20 minutes incubation at room temperature, the wells are washed with diluted washing solution to remove unbound material. A peroxidase conjugated second antibody directed against pistachio proteins is given into the wells and after

Pistachio ELISA Kit ARG80811

20 minutes of incubation the plate is washed again. A substrate solution is added and incubated for 20 minutes, resulting in the development of a blue color. The color development is inhibited by the addition of a stop solution, and the color turns yellow. The yellow color is measured at 450 nm. The concentration of pistachio proteins is directly proportional to the color intensity of the test sample.

MATERIALS PROVIDED & STORAGE INFORMATION

Store the unopened kit at 2-8 °C. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody-coated microplate	12 strips x 8-well	4°C
HRP-antibody Conjugate	15 ml (ready to use)	4°C
Standards (0, 1, 4, 10, 40 ppm)	5 X 1 ml	4°C
10x Extraction and sample dilution buffer	2 X 120 ml	4°C
10x Wash Buffer	60 ml	4°C
TMB substrate	15 ml	4°C (Protect from light)
STOP solution	15 ml	4°C

MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of measuring absorbance at 450nm
- Pipettes and pipette tips
- Deionized or distilled water
- Automated microplate washer (optional)

TECHNICAL HINTS AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Store the kit at 4°C at all times.
- Briefly spin down the HRP-Antibody conjugate before use.
- If crystals are observed in the 10X Wash buffer, Extraction Buffer and Sample diluent buffer, warm to RT (not more than 50°C) until the crystals are completely dissolved.
- Ensure complete reconstitution and dilution of reagents prior to use.
- It is highly recommended that the standards, samples and controls be assayed in duplicates.
- Change pipette tips between the addition of different reagent or samples.
- Samples contain azide cannot be assayed.

SAMPLE COLLECTION & STORAGE INFORMATION

Due to high risk of cross-contamination all applied instruments like applicator, mortar, glass vials etc. have to be cleaned thoroughly before and after each sample. Hazelnut proteins adhere very strongly to different surfaces. In certain cases they can resist a common dishwasher cleaning. To identify possible cross-contamination caused by previous extractions it is strongly recommended to note the sequence of the extractions.

The following sample preparation should be applied for all kinds of samples:

1. To maximize homogeneity and representativeness of the sample

Pistachio ELISA Kit ARG80811

drawing, a minimum of 5 g sample should be pulverized finely in a mortar, impact mill etc.

2. 1 g of the homogenized mixture is suspended in 20 mL of pre-diluted extraction buffer. Afterwards the suspension is incubated for 15 min in a preheated water bath at 60°C. To ensure good homogeneity, the samples should be shaken every two minutes.
3. The samples are centrifuged for 10 minutes at 2500 g. If it is not possible to separate the supernatant from the precipitate completely, the suspension should be filtrated if necessary.
4. 100 µL of particle-free solution are applied per well. If the results of a sample are out of the measuring range, further dilution with the pre-diluted extraction and sample dilution buffer is necessary. The additional dilution has to be considered when calculating the concentration.

The following sample preparation should be applied for liquid samples:

1 mL of liquid sample is diluted in 19 mL of pre-diluted extraction and sample dilution buffer. Afterwards the suspension is incubated for 15 min in a preheated water bath at 60°C. To ensure good homogeneity, the samples should be shaken every two minutes. The process is continued at point 3 of solid sample extraction process.

REAGENT PREPARATION

- **1X Wash buffer:** Dilute 10X wash buffer into distilled water to yield 1X wash buffer.
- **1X Extraction and Sample diluent buffer:** Dilute 10X Extraction and

Sample diluent buffer into distilled water to yield 1X.

ASSAY PROCEDURE

All materials should be equilibrated to room temperature (RT) before use. Standards, samples and controls should be assayed in duplicates.

1. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal it.
2. Add 100 μ l of standards and samples in duplicate into wells.
3. Incubate for 20 minutes at RT.
4. Aspirate each well and wash, repeating the process 2 times for a total 3 washes. Wash by filling each well with 1X wash buffer (350 μ l) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
5. Add 100 μ l of HRP-Antibody Conjugate into each well. Incubate for 20 minutes at RT.
6. Aspirate and wash well as step 4.
7. Add 100 μ l of TMB mixture to each well. Incubate for 20 minutes at room temperature in dark.
8. Add 100 μ l of Stop Solution to each well.
9. Read the OD with a microplate reader at 450 nm immediately.

CALCULATION OF RESULTS


1. Calculate the average absorbance values for each set of standards, controls and patient samples.

Pistachio ELISA Kit ARG80811

- Using linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
- Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
- Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results. The diluted samples must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.

EXAMPLE OF TYPICAL STANDARD CURVE

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

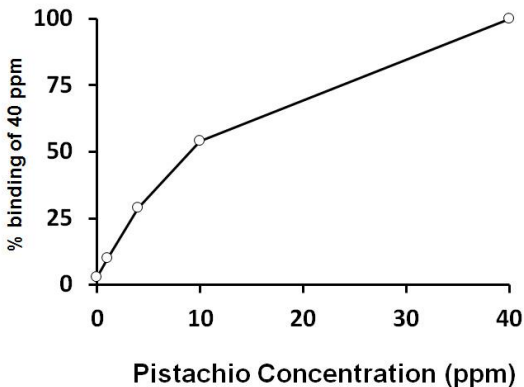

QUALITY ASSURANCE

Sensitivity

The limit of detection (LOD) of the Pistachio test is 0.13 ppm for the standard curve. Validation experiments with common matrices resulted in the following LODs [ppm].

Cookies	0.18
Cereals	0.01
Ice cream	0.20
Chocolate	0.09
Sausage	0.17

The limit of quantification (LOQ) of the Pistachio test is 1 ppm.

Due to the variety of sample matrices and their influence on the blank, results less than the LOQ should be treated as negative.

Specificity

For the following foods no cross-reactivity could be detected:

Almond	Coconut	Plum
Apricot	Cod	Poppy seed
Barley	Corn	Pork meat
Bean	Cow's milk	Potato
Beef	Egg	Pumpkin seed
Bovine gelatin	Guar gum	Rice
Brazil nut	Kiwi	Rye
Carob gum	Lentil	Saccharose
Carrot	Lupin	Sesame
Celery	Macadamia	Shrimp
Cherry	Mustard	Soy
Chestnut	Oats	Soy lecithin
Chicken meat	Pea	Tomato
Chickpea	Peanut	Wheat
Cocoa	Pine seed	

Pistachio ELISA Kit ARG80811

The following cross reactions were determined:

Cashew	12%
Hazelnut	0.017%
Pecan	0.0005%
Sunflower seed	0.0002%
Walnut	0.0008%

Intra-assay and Inter-assay precision

The CV value of intra-assay precision was 6-8% and the CV value of inter-assay precision was 5-12%

Recovery

Cookies	94%
Cereals	96%
Ice cream	89%
Chocolate	81%
Sausage	90%