



# Human IL17F ELISA Kit

Enzyme Immunoassay for the quantification of Human IL17F in Serum,  
plasma and cell culture supernatants

Catalog number: ARG81199

## **TABLE OF CONTENTS**

<b>SECTION</b>	<b>Page</b>
INTRODUCTION .....	3
PRINCIPLE OF THE ASSAY .....	3
MATERIALS PROVIDED & STORAGE INFORMATION .....	4
MATERIALS REQUIRED BUT NOT PROVIDED .....	4
TECHNICAL HINTS AND PRECAUTIONS .....	5
SAMPLE COLLECTION & STORAGE INFORMATION .....	5
REAGENT PREPARATION.....	6
ASSAY PROCEDURE .....	8
CALCULATION OF RESULTS .....	9
EXAMPLE OF TYPICAL STANDARD CURVE .....	10
QUALITY ASSURANCE.....	11

### **MANUFACTURED BY:**

Arigo Biolaboratories Corporation

Address: No. 22, Ln. 227, Gongyuan Rd., Hsinchu City 300, Taiwan

Phone: +886 (3) 562 1738

Fax: +886 (3) 561 3008

Email: [info@arigobio.com](mailto:info@arigobio.com)

### INTRODUCTION

The protein encoded by this gene is a cytokine that shares sequence similarity with IL17. This cytokine is expressed by activated T cells, and has been shown to stimulate the production of several other cytokines, including IL6, IL8, and CSF2/GM-CSF. This cytokine is also found to inhibit the angiogenesis of endothelial cells and induce endothelial cells to produce IL2, TGFB1/TGFB, and monocyte chemoattractant protein-1. [provided by RefSeq, Jul 2008]

Stimulates the production of other cytokines such as IL-6, IL-8 and granulocyte colony-stimulating factor, and can regulate cartilage matrix turnover. Stimulates PBMC and T-cell proliferation. Inhibits angiogenesis. [UniProt]

### PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for IL17F has been pre-coated onto a microtiter plate. Standards or samples are pipetted into the wells and any IL17F present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-conjugated antibody specific for IL17F is added to each well and incubate. Following a washing to remove unbound substances, streptavidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. After washing away any unbound antibody-enzyme reagent, a substrate solution (TMB) is added to the wells and color develops in proportion to the amount of IL17F bound in the initial step. The color development is stopped by the addition of acid and the intensity of the color is measured at a wavelength of 450nm  $\pm$ 2nm. The concentration of IL17F

## Human IL17F ELISA kit ARG81199

---

in the sample is then determined by comparing the O.D of samples to the standard curve.

### MATERIALS PROVIDED & STORAGE INFORMATION

Store the unopened kit at 2-8°C. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody-coated microplate	8 X 12 strips	4°C. Unused strips should be sealed tightly in the air-tight pouch.
Standard (Lyophilized)	2 vials (500 pg/ml)	4°C
10X Standard/Sample diluent	1 X 25 ml	4°C
Antibody conjugate concentrate	1 vial (400 µl)	4°C
Antibody diluent buffer	7 ml (Ready to use)	4°C
HRP-Streptavidin concentrate	2 vials (5 µl)	4°C
HRP-Streptavidin diluent buffer	23 ml (Ready to use)	4°C
200X Wash buffer	10 ml	4°C
TMB substrate	11 ml (Ready to use)	4°C (Protect from light)
STOP solution	11 ml (Ready to use)	4°C
Plate sealer	2 strips	Room temperature

### MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of measuring absorbance at 450nm (optional: read at 610-650 nm as the reference wave length)
- Pipettes and pipette tips
- Deionized or distilled water
- Vortex mixer

## Human IL17F ELISA kit ARG81199

---

- Automated microplate washer (optional)

### TECHNICAL HINTS AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Store the kit at 4°C at all times.
- Briefly spin down the antibody conjugate concentrate and HRP-Streptavidin concentrate before use.
- If crystals are observed in the 200X Wash buffer or Standard/Sample diluent concentrate, warm to RT until the crystals are completely dissolved.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Thoroughly mix the reagents and samples before use by agitation or swirling.
- It is highly recommended that the standards and samples be assayed in duplicates.
- Change pipette tips between the addition of different reagent or samples.
- All reagents should be warmed to room temperature before use.

### SAMPLE COLLECTION & STORAGE INFORMATION

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

**Cell Culture Supernatants** - Remove particulates by centrifugation (1000 X g, 10 min at 2-8°C) and aliquot & store samples at -70°C. Avoid repeated freeze-thaw cycles.

## Human IL17F ELISA kit ARG81199

---

**Serum**- Use a serum separator tube (SST) and allow samples to clot for few minutes before centrifugation (1000 x g) for 10 minutes at 2-8°C. Remove serum and assay immediately or aliquot and store samples at -70°C. Avoid repeated freeze-thaw cycles.

**Plasma** - Collect plasma on ice using EDTA, citrate or heparin as an anticoagulant. Centrifuge (1000 x g) for 30 minutes at 2-8°C within 30 minutes of collection. Collect the supernatants and assay immediately or aliquot and store samples at -70°C. Avoid repeated freeze-thaw cycles.

Note:

- It is recommended that thaw the samples at room temperature and make sure that sample is completely thawed and homogeneous before use. Do not thaw by heating at 37°C or 56°C.
- Avoid using haemolysed or lipemic samples.
- If large amounts of particles are present these should be removed prior to use by centrifugation or filtration.

### REAGENT PREPARATION

- **1X Wash buffer:** Dilute 200X Wash buffer into distilled water to yield 1X Wash buffer (e.g. 10 ml 200X Wash buffer + 1990 ml distilled water). Store the 1X wash buffer at 2-8°C for up to 1 week.
- **1X Antibody conjugate:** Prepare immediately before use, dilute 27.5X antibody conjugate concentrate into 1X antibody diluent buffer with Antibody diluent buffer to yield 1X detection antibody solution (e.g. for 16 wells, add 40 µl Antibody conjugate concentrate into 1060 µl Antibody diluent buffer). Use 1X Antibody conjugate immediately and do

## Human IL17F ELISA kit ARG81199

---


not store.

- **HRP-Streptavidin working solution:** Prepare immediately before use, it is recommended to centrifuge the vial for a few seconds to spin down all the volume at the bottom. Add 0.5 ml HRP-Streptavidin diluent buffer in the vial that contains 5 µl of HRP-Streptavidin concentrate solution, mix completely to get the 1<sup>st</sup> diluted HRP-Streptavidin Solution. Then further dilute the solution 1:66.67 with HRP-Streptavidin diluent buffer to yield 1X HRP-Streptavidin working Solution. (e.g. for 16 wells, add 30 µl of 1<sup>st</sup> diluted HRP-Streptavidin Solution into 2ml HRP-Streptavidin diluent buffer). Use 1X HRP-Streptavidin working Solution immediately and do not store.
- **1X Standard/Sample Diluent Buffer:** Dilute 10X Standard/Sample Diluent Buffer into distilled water to yield 1X Standard/Sample Diluent Buffer (e.g. 25 ml Standard/Sample Diluent Buffer + 225 ml distilled water). Store the 1X Standard/Sample Diluent Buffer at 2-8°C for up to 1 week.
- **Sample:** Serum or plasmas samples have to be diluted 1:2 in Standard/Sample diluent. If the initial assay found samples contain IL17F higher than the highest standard, the samples can be further diluted with Standard/Sample diluent and then re-assay the samples. For the calculation of the concentrations this dilution factor has to be taken into account.  
**(It is recommended to do pre-test to determine the suitable dilution factor).**
- **Standards:** immediately before use, reconstitute the standard with **(volume depend on the lot)** of 1x Standard/Sample diluent to yield a stock

## Human IL17F ELISA kit ARG81199

---

concentration of 500 pg/ml. Mix the reconstituted standard gently by inversion only, and make sure the standard is dissolved completely before making serial dilutions. The 1x Standard/Sample diluent serves as zero standard (0 ng/ml), and the rest of the standard serial dilution can be diluted with 250  $\mu$ l 1x Standard/Sample diluent as according to the suggested concentration below: 500 pg/ml, 250 pg/ml, 125 pg/ml, 62.5 pg/ml, 31.25 pg/ml, 15.625 pg/ml.

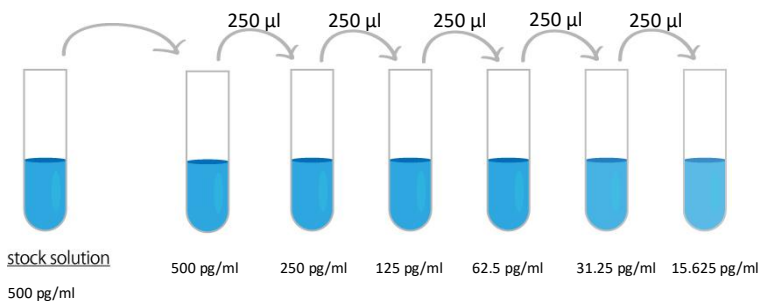

### ASSAY PROCEDURE

All materials should be equilibrated to room temperature (18 - 25°C) before use, each vial should be mixed thoroughly without foaming prior to use. Standards and samples should be assayed in duplicates.

1. Remove excess microplate strips from the plate frame, return them to the foil pouch containing the desiccant pack, and reseal it.
2. Add 100  $\mu$ l of standards, samples and zero standard (Standard/Sample diluent) into wells. Cover wells and incubate for 2 hour at room temperature.



## Human IL17F ELISA kit ARG81199

---

3. Aspirate each well and wash, repeating the process two times for a total three washes. Wash by filling each well with 1× Wash Buffer (300 µl) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
4. Add 50 µl 1X Antibody conjugate into each well. Cover wells and incubate for 1 hour at room temperature.
5. Aspirate each well and wash as step 3.
6. Add 100 µl of 1X HRP-Streptavidin working solution to each well. Cover wells and incubate for 30 minutes at room temperature.
7. Aspirate each well and wash as step 3.
8. Add 100 µl of TMB substrate reagent to each well. Incubate for 10-20 minutes at room temperature in dark.
9. Add 100 µl of Stop Solution to each well. The color of the solution should change from blue to yellow. Gently tap the plate to ensure thorough mixing.
10. Read the OD with a microplate reader at 450 nm immediately. (optional: read at 610-650 nm as the reference wave length)

## CALCULATION OF RESULTS

1. Calculate the average absorbance values for each set of standards, controls and patient samples.
2. Using linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with

## Human IL17F ELISA kit ARG81199


---

absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.

- Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
- Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
- If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.
- Expected serum values: A panel of 20 apparently healthy blood donors was tested for IL17F. All were below the detection level <6 pg/ml.

### EXAMPLE OF TYPICAL STANDARD CURVE

The following data is for demonstration only and cannot be used in place of data generations at the time of assay.

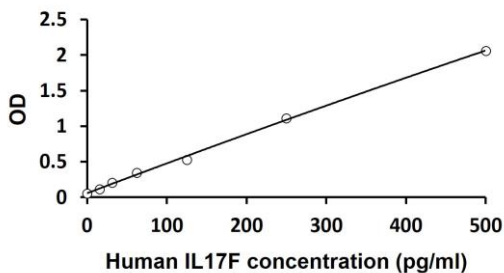

## **QUALITY ASSURANCE**

### **Sensitivity**

The minimum detectable dose (MDD) of Human IL17F ranged from 15.6- 500 pg/ml. The mean MDD was 6 pg/ml.

### **Specificity**

This assay recognizes natural soluble Human IL17F. No significant cross-reactivity or interference with the factors below was observed:

IL17A, IL17B, IL17D, IL17E, IL5, IL23, Perforin.

This kit might cross react to the human IL17A/F heterodimer.

### **Intra-assay and Inter-assay precision**

Intra-assay: 7.13%.

Inter-assay: 7.6%

### **Recovery range:**

Serum: 68-113%, and the overall mean recovery was 89%.