



Human Free Triiodothyronine (fT3) ELISA Kit

Enzyme Immunoassay for the quantitative determination of Free Triiodothyronine (fT3) concentration in Human serum.

Catalog number: ARG82800

Package: 96 wells

For research use only. Not for use in diagnostic procedures.

TABLE OF CONTENTS

SECTION	Page
INTRODUCTION	3
PRINCIPLE OF THE ASSAY	3
MATERIALS PROVIDED & STORAGE INFORMATION.....	4
MATERIALS REQUIRED BUT NOT PROVIDED.....	5
TECHNICAL NOTES AND PRECAUTIONS	5
SAMPLE COLLECTION & STORAGE INFORMATION	6
REAGENT PREPARATION	7
ASSAY PROCEDURE	8
EXAMPLE OF TYPICAL STANDARD VALUES.....	9
CALCULATION OF RESULTS.....	10
QUALITY ASSURANCE	11

MANUFACTURED BY:

Arigo Biolaboratories Corporation

Address: 9F.-7, No. 12, Taiyuan 2nd St., Zhubei City,

Hsinchu County 302082, Taiwan

Phone: +886 (3) 621 8100

Fax: +886 (3) 553 0266

Email: info@arigobio.com

INTRODUCTION

Triiodothyronine, also known as T3, is a thyroid hormone. It affects almost every physiological process in the body, including growth and development, metabolism, body temperature, and heart rate.

L-Triiodothyronine, a thyroid hormone, circulates in blood almost completely bound (>99.5%) to carrier proteins. The main transport protein is thyroxine-binding globulin (TBG). However, only the free (unbound) portion of triiodothyronine is believed to be responsible for the biological action.

T3 is the true hormone. Its effects on target tissues are roughly four times more potent than those of T4. Of the thyroid hormone that is produced, just about 20% is T3, whereas 80% is produced as T4. Roughly 85% of the circulating T3 is later formed in the liver and anterior pituitary by removal of the iodine atom from the carbon atom number five of the outer ring of T4. In any case, the concentration of T3 in the human blood plasma is about one-fortieth that of T4. The half-life of T3 is about 2.5 days. The half-life of T4 is about 6.5 days. [Provided by Wikipedia: Triiodothyronine]

PRINCIPLE OF THE ASSAY

This assay employs the competitive quantitative enzyme immunoassay technique. A highly specific antibody for Free Triiodothyronine has been pre-coated onto a microplate. Free Triiodothyronine (fT3) containing samples, Controls or Standards and fT3-HRP conjugate are given into the wells of the microtiter plate. Enzyme labeled and free Triiodothyronine compete for the

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

antibody binding sites. After incubation at room temperature, the wells are washed with diluted Wash Buffer to remove unbound material. Then TMB substrate is added to the wells and color develops in inversely proportion to the amount of fT3 present in the samples. The color development is stopped by the addition of STOP solution and the intensity of the color is measured at a wavelength of 450 nm. The concentration of fT3 in the samples is then determined by comparing the O.D of samples to the standard curve.

MATERIALS PROVIDED & STORAGE INFORMATION

Store all other components at 2-8°C. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody Coated microplate	8 X 12 strips	4°C
Standards A to F (0, 2, 4, 8, 16, 40 pg/mL)	0.5 mL each (ready to use)	4°C
Control 1	0.5 mL each (4.67 ng/ml; accept range: 3.42-5.70 pg/ml)	4°C
Control 2	0.5 mL each (8.66 ng/ml; accept range: 6.38-10.60 pg/ml)	4°C
Diluent Buffer	15 mL (ready to use)	4°C
50X fT3-HRP Conjugate	300 µL	4°C
10X Wash Buffer	50 mL	4°C
TMB substrate	16 mL (ready to use)	4°C (protect from light)
STOP solution	6 mL (ready to use)	4°C

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of reading at 450 nm (620 nm as optional reference wave length)
- Deionized or distilled water
- Mixer or Ultra-Turrax
- Microplate shaker
- Temperature control incubator (37°C)
- Pipettes and pipette tips
- Microtiter plate washer (recommended)

TECHNICAL NOTES AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Store the kit at 2-8°C at all times.
- Prior to beginning the assay procedure, bring all reagents and required number of strips to room temperature (20-25°C) before use.
- Avoid air bubbles in the wells as this could result in lower binding efficiency and higher CV% of duplicate reading.
- Briefly spin down the all vials before use.
- If crystals are observed in the 10X Wash Buffer, warm to 37°C until the crystals are completely dissolved.
- Minimize lag time between wash steps to ensure the plate does not become completely dry during the assay.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Take care not to contaminate the TMB Substrate. Do not expose the TMB

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

solution to glass, foil or metal. If the solution is blue before use, DO NOT USE IT.

- Do NOT return leftover TMB Substrate to bottle. Do NOT contaminate the unused TMB Substrate. If the solution is blue before use, DO NOT USE IT.
- Change pipette tips between the addition of different reagent or samples.
- Taping the well strips together with lab tape can be done as an extra precaution to avoid plate strips from coming loose during the procedure.
- Include a standard curve and controls each time the assay is performed.
- Run both standards and samples in at least duplicates (triplicate is recommended).

SAMPLE COLLECTION & STORAGE INFORMATION

The following recommendations are only guidelines and may be altered to optimize or complement the user's experimental design.

Serum: Collect blood in a tube with no anticoagulant. Allow the blood to clot at room temperature for 30 minutes. Centrifuge at 2500 x g for 20 minutes.

Note:

1. Do not use haemolytic, icteric or lipaemic specimens.
2. Avoid disturbing the white buffy layer when collection serum/plasma sample.
3. Samples containing sodium azide should not be used in the assay.
4. Specimens should be capped and may be stored for up to 24 hours at 2-8°C prior to assaying. Specimens stored for a longer time (up to 3 months) should be frozen only once at -20°C prior to assay. Thawed samples should be inverted several times prior to testing.

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

5. Sample reading higher than Standard F (40 pg/mL) should be reported as > 40 pg/mL, and sample should not be diluted. Dilution will alter the existing equilibrium and may lead to false results.
6. The interpretation of fT3 results can be complicated by a variety of drugs, severe nonthyroidal illness and some rare conditions such as familial dysalbuminemic hyperthyroxinemia (FDH). For diagnostic purposes, the results of this assay should always be used in combination with the clinical examination, medical history and other findings.

REAGENT PREPARATION

- **1X Wash Buffer:** Dilute 10X Wash Buffer into distilled water to yield 1X Wash Buffer. (E.g., add 50 mL of 10X Wash Buffer into 450 mL of distilled water to a final volume of 500 mL) The 1X Wash Buffer is stable for up to 4 weeks at 2-8°C.
- **1X fT3-HRP Conjugate:** Dilute 1:50 in Diluent Buffer before use (E.g. 40 µL of fT3-HRP Conjugate in 2 mL of Diluent Buffer). If the whole plate is to be used dilute 240 µL of HRP in 12 mL of Diluent Buffer. Discard any that is left over.

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

ASSAY PROCEDURE


All materials should be equilibrated to room temperature (RT, 20-25°C) before use. Standards and samples should be assayed in duplicates.

1. Add **25 µL** of **Standards, Controls and samples** into the appropriate wells of the Antibody Coated Microplate.
2. Add **100 µL** of **fT3-HRP Conjugate** into all wells.
3. Incubate at **37°C** for **60 minutes** on a microplate shaker.
4. Aspirate each well and wash, repeating the process 2 times for a total **3 washes**. Wash by filling each well with **1× Wash Buffer (300 µL)** using a squirt bottle, manifold dispenser, or autowasher. Then complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
5. Add **150 µL** of **TMB Substrate** to each well, including the blank wells. Incubate in the dark for **10-15 minutes** at **37°C** on a microplate shaker.
6. Immediately Add **50 µL** of **Stop Solution** to each well, including the blank wells. The color of the solution should change from blue to yellow.
7. Read the OD with a microplate reader at **450 nm** immediately. (optional: read at 620 nm as reference wavelength) It is recommended reading the absorbance **within 20 minutes** after adding the stop solution.

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

EXAMPLE OF TYPICAL STANDARD VALUES

The following figures demonstrate typical results with the Human Free Triiodothyronine (fT3) ELISA Kit. One should use the data below for reference only. This data should not be used to interpret actual results.

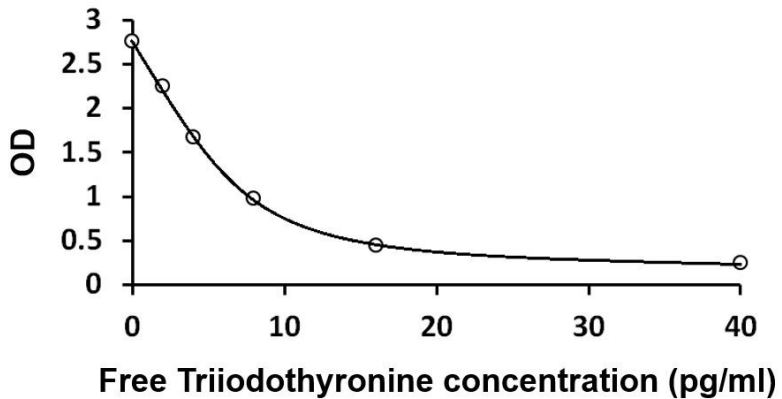

Human Free Triiodothyronine (ft3) ELISA kit ARG82800

CALCULATION OF RESULTS

1. Calculate the average absorbance values for each set of Controls, standards and samples.
2. Using log-log, semi-log or linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
3. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
4. arigo provides GainData®, an in-house development ELISA data calculator, for ELISA data result analysis. Please refer our GainData® website for details. (<https://www.arigobio.com/elisa-analysis>)
5. Sample reading higher than Standard F (40 pg/mL) should be reported as > 40 pg/mL.
6. The ft3-HRP Conjugate employed in this assay system has shown no substantial binding properties towards thyroxine-binding globulin (TBG) or human serum albumin (HSA). The binding sites on the microplates are designed to be of a low binding-capacity in order not to disturb the equilibrium between T3 and its carrying proteins. The assay is carried out under normal physiological conditions of pH, temperature and ionic strength.

Human Free Triiodothyronine (fT3) ELISA kit ARG82800

QUALITY ASSURANCE

Sensitivity

The sensitivity of the Human Free Triiodothyronine (fT3) ELISA kit is 0.3 pg/mL.

Specificity

Substance	Cross Reactivity (%)
L-Triiodothyronine	100
D-Triiodothyronine	34
Triiodothyropropionic acid	20
Diiodo-D-thyronine	0.5
D-Thyroxine	0.3
L-Thyroxine	0.9

The following compounds were tested but cross-reacted at less than 0.1%: Diiodotyrosine, Iodotyrosine, Phenytoin, Sodium Salicylate and r-Triiodothyronine.

Intra-assay and Inter-assay precision

The CV value of intra-assay precision was 3.5-9.7% and CV value of inter-assay precision was 7.8-8.6%.

Expected Normal Values

Group	N	Mean (pg / mL)	Central 95% range (pg / mL)
Healthy Adults	44	3.7	2.2-5.3