



Mouse TNF alpha ELISA Kit

Mouse TNF alpha ELISA Kit is an Enzyme Immunoassay kit for the quantification of Mouse TNF alpha in serum, plasma and Cell culture supernatants.

Catalog number: ARG82989

Package: 96 wells

Lot: 354558

For research use only. Not for use in diagnostic procedures.

TABLE OF CONTENTS

SECTION	Page
INTRODUCTION	3
PRINCIPLE OF THE ASSAY	4
MATERIALS PROVIDED & STORAGE INFORMATION.....	5
MATERIALS REQUIRED BUT NOT PROVIDED.....	5
TECHNICAL NOTES AND PRECAUTIONS	6
SAMPLE COLLECTION & STORAGE INFORMATION	7
REAGENT PREPARATION	8
ASSAY PROCEDURE	10
CALCULATION OF RESULTS.....	11
EXAMPLE OF TYPICAL STANDARD CURVE.....	12

MANUFACTURED BY:

Arigo Biolaboratories Corporation

Address: No. 22, Ln. 227, Gongyuan Rd., Hsinchu City 300, Taiwan

Phone: +886 (3) 562 1738

Fax: +886 (3) 561 3008

Email: info@arigobio.com

INTRODUCTION

Tumor necrosis factor (TNF, cachexin, or cachectin; often called tumor necrosis factor alpha or TNF- α) is an adipokine and a cytokine. TNF is a member of the TNF superfamily, which consists of various transmembrane proteins with a homologous TNF domain.

As an adipokine, TNF promotes insulin resistance, and is associated with obesity-induced type 2 diabetes. As a cytokine, TNF is used by the immune system for cell signaling. If macrophages (certain white blood cells) detect an infection, they release TNF to alert other immune system cells as part of an inflammatory response.

TNF signaling occurs through two receptors: TNFR1 and TNFR2. TNFR1 is constitutively expressed on most cell types, whereas TNFR2 is restricted primarily to endothelial, epithelial, and subsets of immune cells. TNFR1 signaling tends to be pro-inflammatory and apoptotic, whereas TNFR2 signaling is anti-inflammatory and promotes cell proliferation. Suppression of TNFR1 signaling has been important for treatment of autoimmune disease, whereas TNFR2 signaling promotes wound healing. [Provide by Wikipedia: Tumor necrosis factor]

PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. An antibody specific for Mouse TNF alpha has been pre-coated onto a microtiter plate. Standards or samples are pipetted into the wells and any TNF alpha present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-conjugated antibody specific for Mouse TNF alpha is added to each well and incubated. Following a washing to remove unbound substances, streptavidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. After washing away any unbound antibody-enzyme reagent, a substrate solution (TMB) is added to the wells and color develops in proportion to the amount of Mouse TNF alpha bound in the initial step. The color development is stopped by the addition of acid and the intensity of the color is measured at a wavelength of 450nm. The concentration of Mouse TNF alpha in the sample is then determined by comparing the O.D of samples to the standard curve.

Mouse TNF alpha ELISA Kit ARG82989

MATERIALS PROVIDED & STORAGE INFORMATION

Upon received, store 100X Antibody Conjugate concentrate at $\leq -20^{\circ}\text{C}$. Store other component at $2-8^{\circ}\text{C}$ at all times. Use the kit before expiration date.

Component	Quantity	Storage information
Antibody Coated Microplate	8 x 12 strips	4°C .
Standard (Lyophilized)	3 X 2 ng/vial	4°C
Standard / Sample Diluent Buffer	20 mL (Ready to use)	4°C
100X Antibody Conjugate Concentrate	1 vial (120 μL)	-20°C
1000X HRP-Streptavidin Solution	1 vial (15 μL)	4°C (Protect from light)
Antibody Diluent Buffer	35 mL (Ready to use)	4°C
10X Wash Buffer	50 mL	4°C
TMB Substrate	12 mL (Ready to use)	4°C (Protect from light)
Stop Solution	12 mL (Ready to use)	4°C
Plate sealer	4 adhesive strips	Room temperature

MATERIALS REQUIRED BUT NOT PROVIDED

- Microplate reader capable of reading at O.D. 450 nm
- Centrifuge and centrifuge tube
- Deionized or Distilled water
- Pipettes, pipette tips and Multichannel micropipette reservoir
- Automated microplate washer (optional)

TECHNICAL NOTES AND PRECAUTIONS

- Wear protective gloves, clothing, eye, and face protection especially while handling blood or body fluid samples.
- Upon received, store 100X Antibody Conjugate concentrate at $\leq -20^{\circ}\text{C}$. Store other component at $2-8^{\circ}\text{C}$ at all times.
- Prior to beginning the assay procedure, bring all reagents and required number of strips to room temperature.
- Avoid air bubbles in the wells as this could result in lower binding efficiency and higher CV% of duplicate reading.
- Briefly spin down the all vials before use.
- If crystals are observed in the 10X Wash Buffer, warm to 37°C until the crystals are completely dissolved.
- Minimize lag time between wash steps to ensure the plate does not become completely dry during the assay.
- Ensure complete reconstitution and dilution of reagents prior to use.
- Take care not to contaminate the TMB Substrate. Do not expose the TMB solution to glass, foil or metal. Do NOT return leftover TMB Substrate to bottle. Do NOT contaminate the unused TMB Substrate. If the solution is blue before use, DO NOT USE IT.
- Change pipette tips between the addition of different reagent or samples.
- Taping the well strips together with lab tape can be done as an extra precaution to avoid plate strips from coming loose during the procedure.
- Include a standard curve each time the assay is performed.
- Run both standards and samples in at least duplicates.

SAMPLE COLLECTION & STORAGE INFORMATION

The sample collection and storage conditions listed below are intended as general guidelines. Sample stability has not been evaluated.

Cell Culture Supernatants - Remove particulates by centrifugation for 10 min at 1500 x g at 4°C and aliquot & store samples at -20°C for up to 1 month or -80°C for up to 6 months. Avoid repeated freeze-thaw cycles.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Collect serum and assay immediately or aliquot & store samples at -20°C for up to 1 month or at -80°C for up to 6 months. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA or heparin as an anticoagulant. Centrifuge for 15 minutes at 1000 x g. within 30 minutes of collection. Collect the supernatants and assay immediately or aliquot and store samples at -20°C for up to 1 month or -80°C for up to 6 months. Avoid repeated freeze-thaw cycles.

Note:

- Do not use haemolytic, icteric or lipaemic specimens.
- Samples containing sodium azide should not be used in the assay.

REAGENT PREPARATION

- **1X Wash Buffer:** Dilute **10X** Wash Buffer into 1X distilled water to yield 1X Wash Buffer (E.g., add 50 mL of 10X Wash Buffer into 450 mL of distilled water to a final volume of 500 mL).
The diluted 1X Wash Buffer is stable for 4 weeks at 2°C to 8°C.
- **1X Antibody Conjugate:** 20 minutes before use, dilute **100X** Antibody Conjugate concentrate into **Antibody Diluent Buffer** to yield 1X Antibody Conjugate.
- **1X HRP-Streptavidin Solution:** 20 minutes before use, dilute **1000X** HRP-Streptavidin Solution into **Antibody Diluent Buffer** to yield 1X HRP-Streptavidin Solution. Keep diluted HRP-Streptavidin Solution in dark before use.
- **Sample:** Diluent serum and plasma samples with equal volume of **Standard / Sample Diluent Buffer** before assay (1:1, dilution factor=2). If the initial assay found samples contain proteins higher than the highest standard, the samples can be diluted with Standard / Sample Diluent Buffer and then re-assay the samples. For the calculation of the concentrations this dilution factor has to be taken into account. Cell culture supernatants could be assayed directly. (It is recommended to do pre-test to determine the suitable dilution factor).
- **Standard:** Centrifuge the un-reconstituted standard at 6000 x g for 1 minute to bring down the material prior to open the vial. Add **1 ml** of **Standard / Sample Diluent Buffer** to a Standard vial to make the high standard concentration of 2000 pg/mL and brief vortex for few seconds

Mouse TNF alpha ELISA Kit ARG82989

(Do not induce foaming) and allow it to sit for 15 minutes. Make sure the standard is dissolved completely before making serial dilutions. The Standard / Sample Diluent Buffer serves as zero standard (0 pg/ml), and the rest of the standard serial dilution can be diluted with Standard / Sample Diluent Buffer. Diluted the standard as below:

Standard tube	TNF alpha (pg/mL)	Standard / Sample Diluent Buffer (μ L)	Standard (μ L)
S1	2000	0	1000 (2000 pg/mL Standard Stock)
S2	1000	500	500 of S1
S3	500	500	500 of S2
S4	250	500	500 of S3
S5	125	500	500 of S4
S6	62.5	500	500 of S5
S7	31.25	500	500 of S6
S0	0	500	0

Note: Working standard should be prepared immediately prior to use.

ASSAY PROCEDURE

All materials should be equilibrated to room temperature (RT, 20-25°C) before use. Standards and samples should be assayed in duplicates.

1. Add **100 µL** of **diluted samples** or **each diluted Standard** into respective wells of the 96-well plate.
2. Cover the plate and incubate for **2 hours** at **room temperature**.
3. Aspirate each well and wash, repeating the process 3 time for a **total 4 washes**. Wash by filling each well with **1X Wash Buffer (300 µL)** using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating, decanting or blotting against clean paper towels.
4. Add **100 µL** of **1X Antibody Conjugate** to each well.
5. Cover the plate and incubate for **1 hour** at **room temperature**.
6. Aspirate each well and **wash plate as step 3**.
7. Add **100 µL** of **1X HRP-Streptavidin Solution** to each well.
8. Cover the plate and incubate for **1 hour** at **room temperature** in the dark.
9. Aspirate each well and **wash plate as step 3**.
10. Add **100 µL** of **TMB Substrate** in each well.
11. Incubate for **10-20 mins** at **room temperature** in the dark.
12. Add **100 µL** of **Stop Solution** to each well to stop the reaction.
13. Read the absorbance with a plate reader at **O.D. 450 nm**. It is recommended reading the absorbance within 30 minutes after adding the stop solution.


CALCULATION OF RESULTS

1. Calculate the average absorbance values for each set of standards, control and samples.
2. Using log-log, semi-log or linear graph paper, construct a standard curve by plotting the mean absorbance obtained from each standard against its concentration with absorbance value on the vertical (Y) axis and concentration on the horizontal (X) axis.
3. Using the mean absorbance value for each sample determine the corresponding concentration from the standard curve.
4. Automated method: The results in the IFU have been calculated automatically using a 4 PL (4 Parameter Logistics) curve fit. 4 Parameter Logistics is the preferred method. Other data reduction functions may give slightly different results.
5. arigo provides GainData®, an in-house development ELISA data calculator, for ELISA data result analysis. Please refer our GainData® website for details. (<https://www.arigobio.com/elisa-analysis>)
6. If the samples have been diluted, the concentration read from the standard curve must be further converted by the appropriate dilution factor according to the sample preparation procedure as described above.

Mouse TNF alpha ELISA Kit ARG82989

EXAMPLE OF TYPICAL STANDARD CURVE

The following figures demonstrate typical results with the Mouse TNF alpha ELISA Kit. One should use the data below for demonstration only and cannot be used in place of data generations at the time of assay.

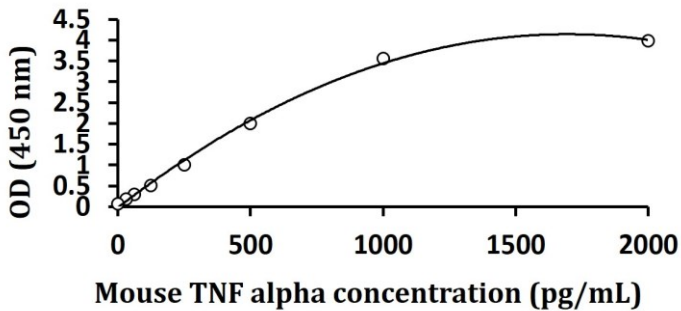

QUALITY ASSURANCE

Sensitivity

15.6 pg/ml

Assay Range

31.25 – 2000 pg/ml